


Information on the transport and storage of ROMA Environmental Simulation and Test chambers

Dear Customer,

With this delivery you are receiving an environmental simulation and test chamber from Romakowski GmbH & Co.KG. Prior to shipment the chamber was subjected to a quality inspection and thus complies with the technical and visual specifications agreed upon. For this to continue to be the case, the following instructions on transport and storage of ROMA environmental simulation and test chambers must be followed:

<p>General information</p>	<p>Work with particular care when unloading and storing, and observe the following safety instructions!</p> <p>The installation and operating instructions must be followed!</p> <p>Avoid damaging the housing.</p>
<p>Transport and shipment</p>	<p>The truck driver shares the responsibility for the correct loading of the truck and proper transportation.</p> <p><u>Only</u> the lashing and attachment points marked in sketch 1 are to be used for securing loads.</p> <p>A careful visual inspection must be carried out prior to unloading when goods are accepted.</p> <p>Any damage or missing accessories must be immediately entered in the shipping documents and reported to Romakowski GmbH & Co. KG without delay. In the event of discrepancies in the scope of delivery or damage, do not commence operation of the housing.</p>
<p>Unloading</p>	<p>To avoid damage to the chambers, during unloading only the specified attachment points are to be used (see sketch 1).</p> <p>Appropriate fastening material and lifting beams must be used for unloading (see sketch 2)!</p> <p>Lifting may only be carried out on the steel frame when unloading with a forklift truck.</p> <p>Ensure that the forks of the forklift truck are sufficiently long!</p> <p>The housing is packed in a special protective foil and the foil should only be removed after transportation to the specified destination.</p> <p>Check the underbody of the chamber for any damage. While doing so, it is forbidden to stand under suspended loads!</p> <p>After unloading, check the chamber or optional accessories for completeness and possible damage.</p>
<p>Storage</p>	<p>The housing must be stored on a flat surface in a well-ventilated and dry location.</p> <p>The packing foil must be removed shortly after delivery to avoid condensation buildup.</p> <p>The protective foil on the panels must be completely removed at the latest three months after delivery. During this period the chamber must be protected from exposure to direct sunlight.</p>

Sketch 1: Fastening and attachment points

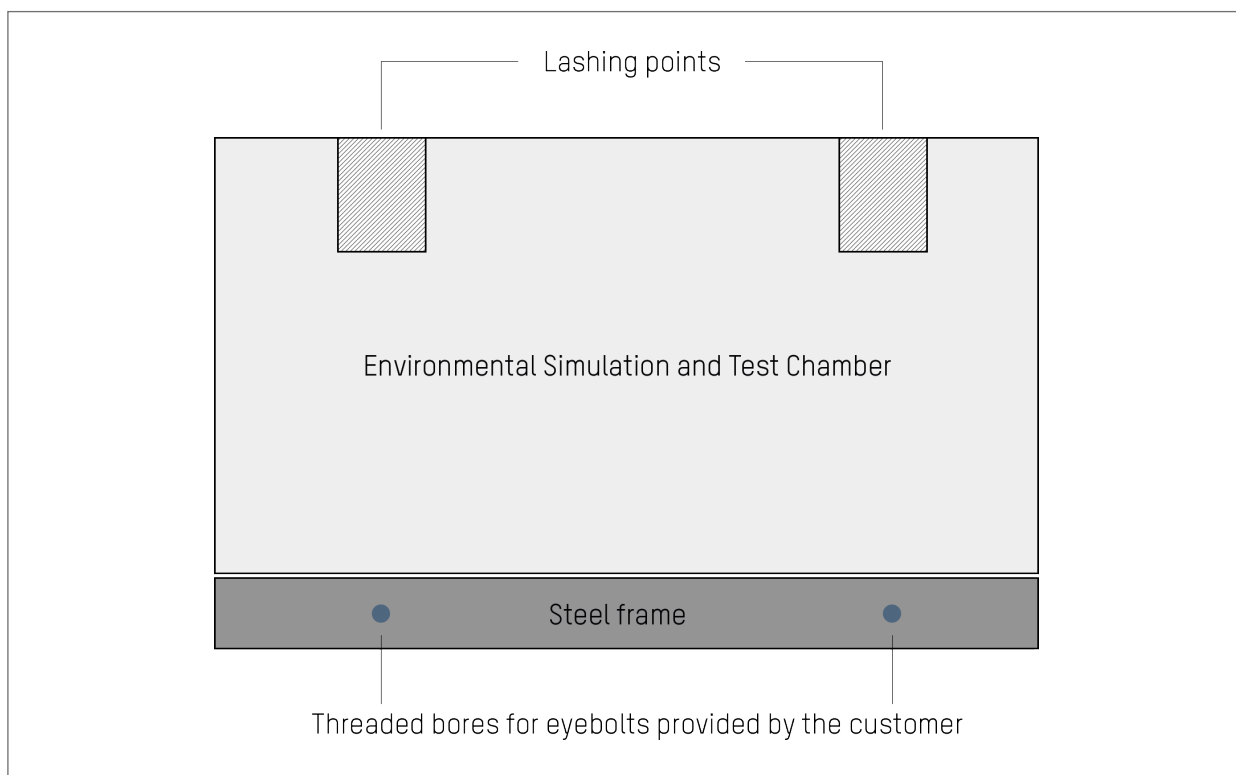

Sketch 2: The use of fastening material

